MOLQ Express Lab

*Free Home Sample Collection 9999 778 778

Download "MOLQ" App on

Book a Test Online www.molq.in

Medical ID	011705270045	Date of Report	2017/5/28

Basic Information

Name	**MRS. JYOTI**
Date of Birth	07/11/1987
Age	29
Weight(Kg)	38.2
Race	ASIAN
Number of Child	1
Smoke or not	FALSE

Ultrasonic Image

u-Gestational weeks	Week		Day
Calculating Method	ByLMP		
Date of Test			
BPD(mm)			
CRL(mm)			
Nasal Bone	FALSE		
		MoM	***Cut-off***
NT(mm)	1.1		<=2.5

Serological test

Date of Test	28/05/2017 00:00	***r-Gestational weeks***	12	Week	0 Day

Parameter	***Result***	***Unit***	***MoM***	***Cut-off***
f-B-HCG	163.4	ng/ml	2.3	<=2.11
PAPPA	8603.49	mIU/L	1.76	>0.25

Risk

Risk of Age	1:1000
Risk of Trisomy 21	1:2320
Risk of Trisomy 18	1:1000000
Risk of NTD	

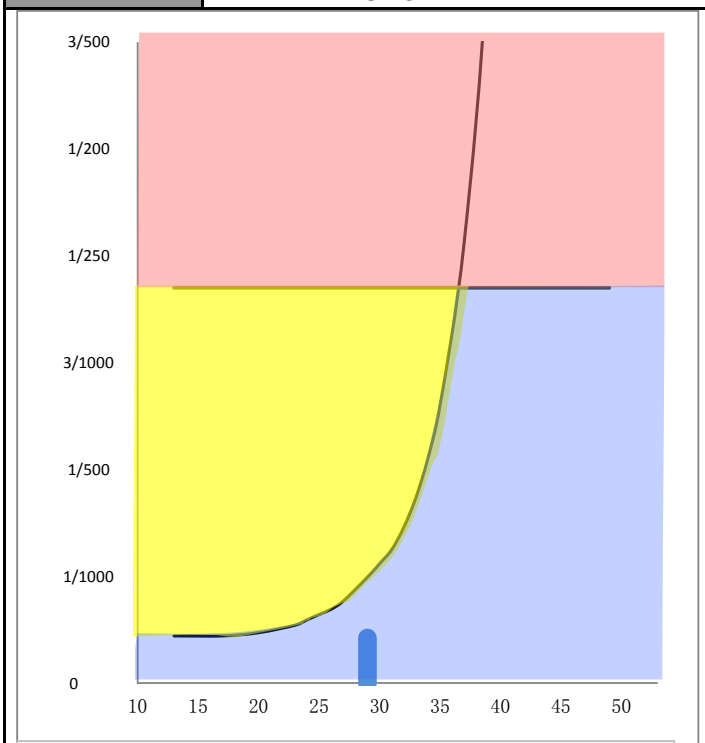

Apple Tree Prenatal Screen software. v20131216

Risks are calculated based on APPLETREE Database with the serological test and Ultrasonic image. Reference to the doctor only.

Down Syndrome

The Down Syndrome result 1:2320 is less than the threshold value 1:600, while Down Syndrome is at low risk.

Edward Syndrome

The Edward Syndrome result 1:1000000 is less than the threshold value 1:600, while Edward Syndrome is at low risk.

NTD